


CoaguChek® XS Plus

Refreshed design for reliable coagulation testing at the point of care.

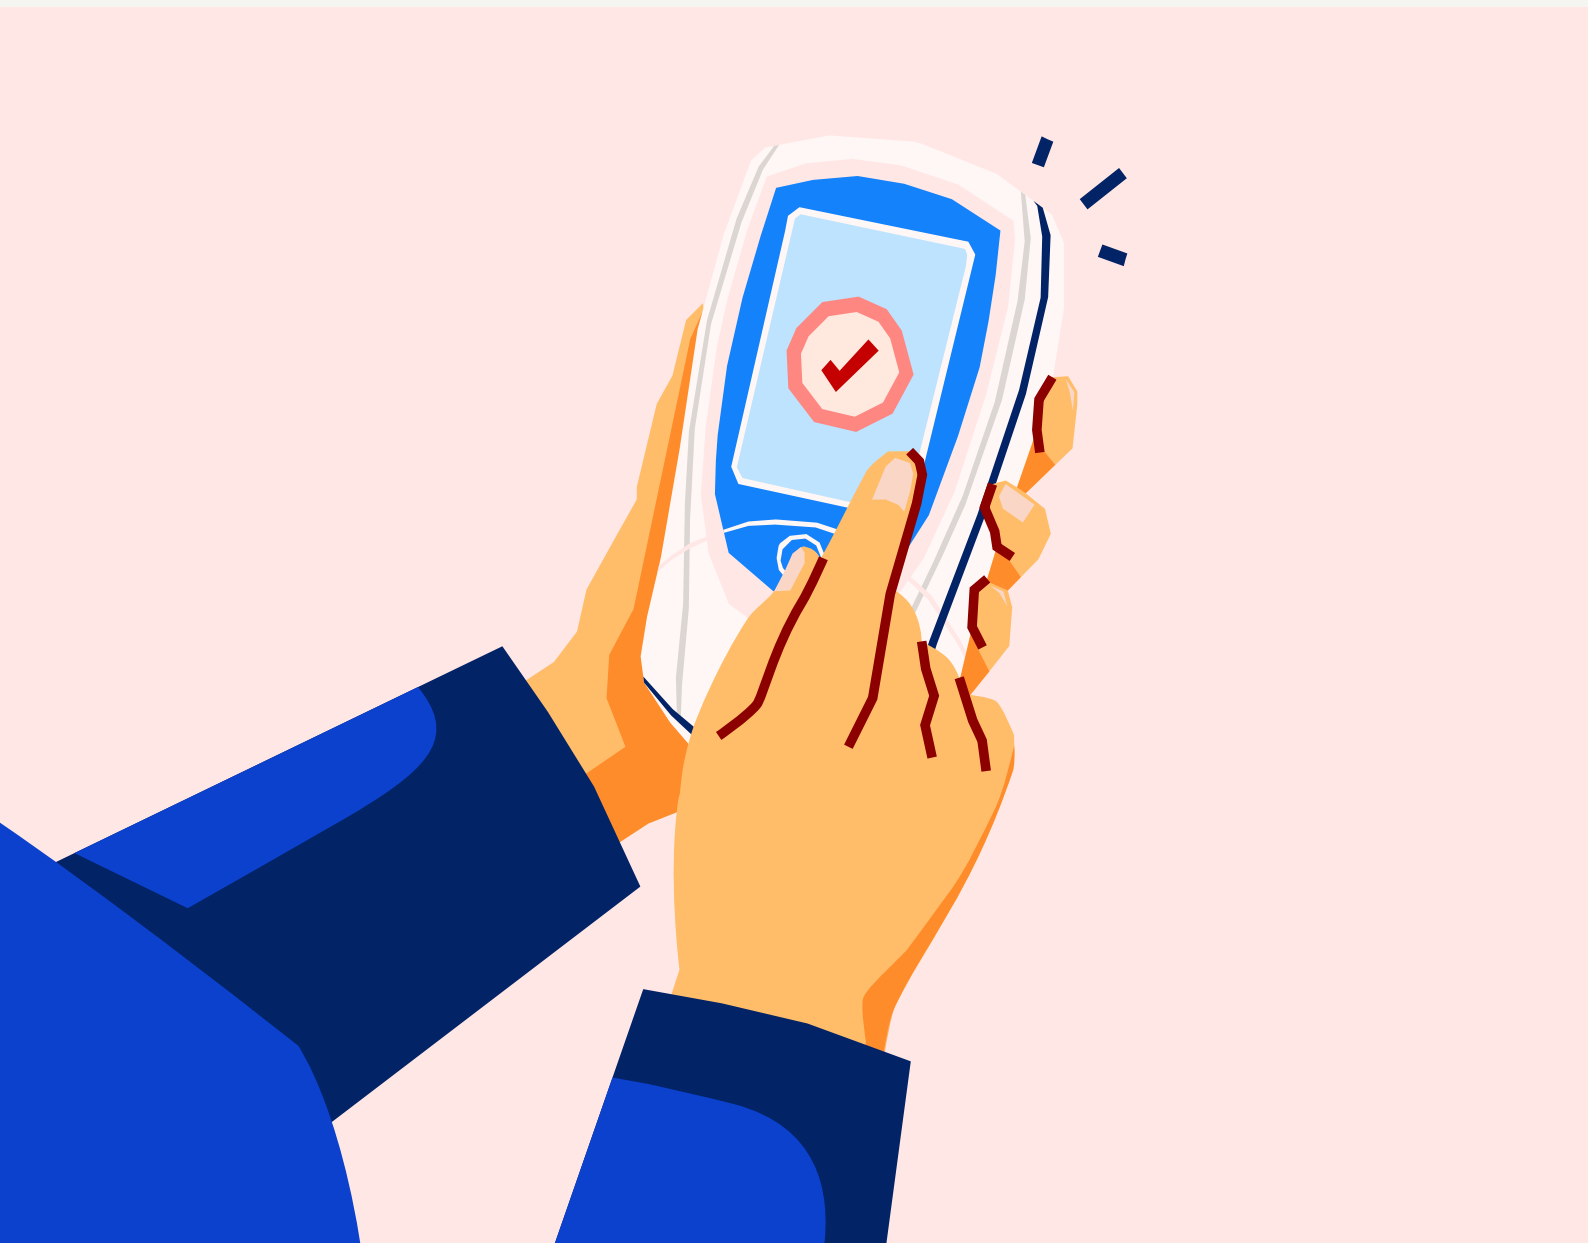


Get immediate,
actionable results
at all points of care.

CoaguChek® XS Plus system is the clinically vital point-of-care coagulation testing device, delivering laboratory-comparable PT/INR results in approximately 1 minute.¹

Cut down time to result and create workflow efficiencies with new features now available on the CoaguChek XS Plus

- Save time and reduce manual entry error for operator IDs, patient IDs, and QC materials with a built-in barcode scanner.
- Reduce downtime and simplify inventory management with the rechargeable battery pack, eliminating the need to acquire, store, track, and replace disposable batteries.
- Enhance the user experience and workflow with the improved, interactive touchscreen display.

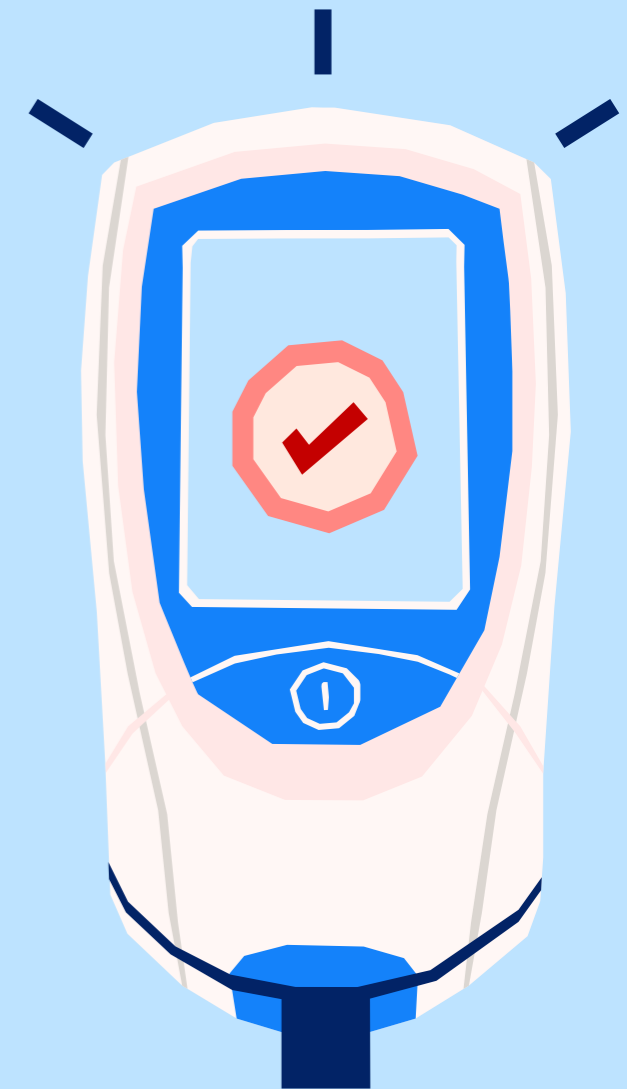

Critical information is available when and where it's needed most.



In Anticoagulation Clinics

- Assess the use of vitamin K antagonists and support patients' anticoagulation therapy treatment.³
- Use rapid PT/INR results to guide and manage patients' anticoagulation therapy and treatment plans.



In the Hospital and Specialty Care Centers

- Monitor PT/INR result trends for anticoagulation therapy patients preparing to undergo cardiovascular surgery.²
- Assess coagulation status of patients on anticoagulation therapy to minimize treatment delay.³



In Primary Care Physicians' Offices

- Use rapid PT/INR results to make warfarin dosage adjustments during patients' appointments without waiting for an external lab result.




Home Healthcare and Nursing Homes

- Conveniently perform PT/INR testing on patients who are homebound reducing the need for them to travel to an anticoagulation clinic.



A clinically vital tool for better patient management.

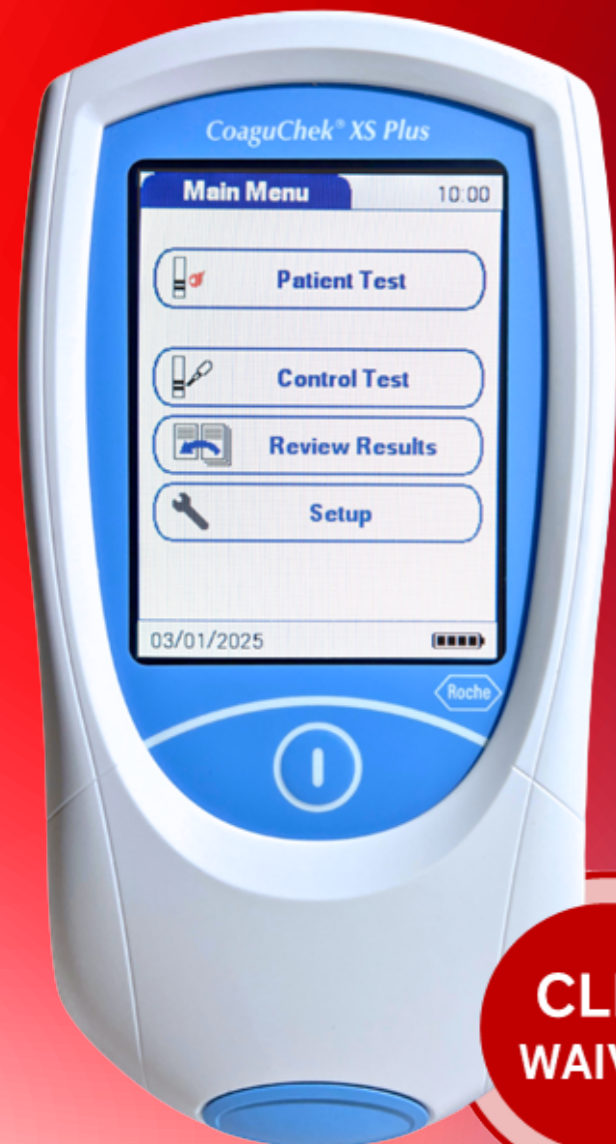

**CLIA
WAIVED**



INR monitoring with CoaguChek means patients no longer have to wait for results from labs, which allows you greater ability to test and monitor your patients.^{1,4} In fact, more frequent testing has been shown to result in more patients achieving INR stability.^{4,5}

- 01 **Accurate results in 1 minute¹**
Confidence from the start.
- 02 **Barcode scanning**
Frees up manual time for clinicians and patients.
- 03 **Connectivity with your data management systems**
Enables data transfer via handheld base unit.
- 04 **Rechargeable battery pack**
Supports continuous use without battery swaps.
- 05 **Supports better care^{1,2}**
Improve time in therapeutic range (TTR).
- 06 **User-friendly touch screen**
Enhanced interface for intuitive on-screen navigation.



System specifications⁶

Measuring range INR	0.8 – 8.0
Sample type	Capillary or fresh, non-anticoagulated venous whole blood
Sample size	≥ 8 µL
Memory	<ul style="list-style-type: none"> • Patient list with up to 4000 Patient IDs with corresponding 2nd and 3rd IDs • Operator list with up to 5000 Operator IDs with corresponding 2nd ID • 2000 patient and 500 QC results with date and time
Interface	Touch screen and barcode scanner
Power	<ul style="list-style-type: none"> • Universal Battery Pack for the CoaguChek XS Plus meter • Power supply adapter: Input 100-240 V AC / 50-60 Hz / 1.2 A
Size	187 x 97 x 43 mm
Weight	280 g (without battery pack)

References

- ¹ CoaguChek® XS PT Test Package Insert (05967694001-v13.0). Indianapolis, IN Roche Diagnostics Corporation; last updated: 2024.
- ² Theusinger OM, Stein P, Levy JH. Point of care and factor concentrate-based coagulation algorithms. *Transfus Med Hemother*. 2015;42:115-121.
- ³ Rooney KD, Schilling UM. Point-of-care testing in the overcrowded emergency department – can it make a difference? *Crit Care*. 2014;18:692.
- ⁴ Ward A, Tompson A, Fitzmaurice D, Sutton S, Perera R, Heneghan C. Cohort study of Anticoagulation Self-Monitoring (CASM): a prospective study of its effectiveness in the community. *Br J Gen Pract*. 2015;65(636):e428-437.
- ⁵ Khan TI, Kamali F, Kesteven P, Avery P, Wynne H. The value of education and self-monitoring in the management of warfarin therapy in older patients with unstable control of anticoagulation. *Br J Haematol*. 2004;126(4):557-654.
- ⁶ CoaguChek® XS Plus [Operator's Manual]. Rotkreuz, Switzerland: Roche; 2025.

COAGUCHEK is a trademark of Roche.

© 2025 Roche

MC-US-17781

Published by

Roche Diagnostics

9115 Hague Rd.

Indianapolis, IN 46256

diagnostics.roche.com
